

CRITICAL CURRENT MEASURING SYSTEM



The HTS-110 8 T Electrical Transport Measuring System provides automated measurement of electrical transport properties as a function of magnetic field, field angle and temperature. Completely cryogen-free $I_c(T, B, \theta)$ to over 800 A, with sample cooling to $T < 20$ K.

Applications

- Critical current in full-size superconducting wire sample
- $I_c(T, B, \theta)$
- n-value
- $R(T)$
- 1G, 2G, MgB

2

Features

- 0-8 T variable field (bipolar)
- Dedicated sample cooler using flowing He gas for high cooling capacity; Sample T from < 20 K to 300 K
- Sample rotation 0-360°
- All measurement hardware including power supplies and meters
- Software suite for full automated control, LabVIEW- based

Easy to use

- Complete automated measurement system
- Entirely cryogen-free operation; no handling of liquid helium or nitrogen, even for cool down
- Magnet safety monitoring electronics standard
- Rapid sample exchange and cooling

Easy to site

- Low fringe field
- Compressors can be sited remotely (up to 10m)
- All measurement electronics mounted in movable rack




HTS-110
1B Quadrant Drive, Waiwhetu
Lower Hutt 5010, New Zealand

☎ +64 4 570 8880
✉ info@hts-110.com
🌐 nz.linkedin.com/company/hts-110



CRITICAL CURRENT MEASURING SYSTEM

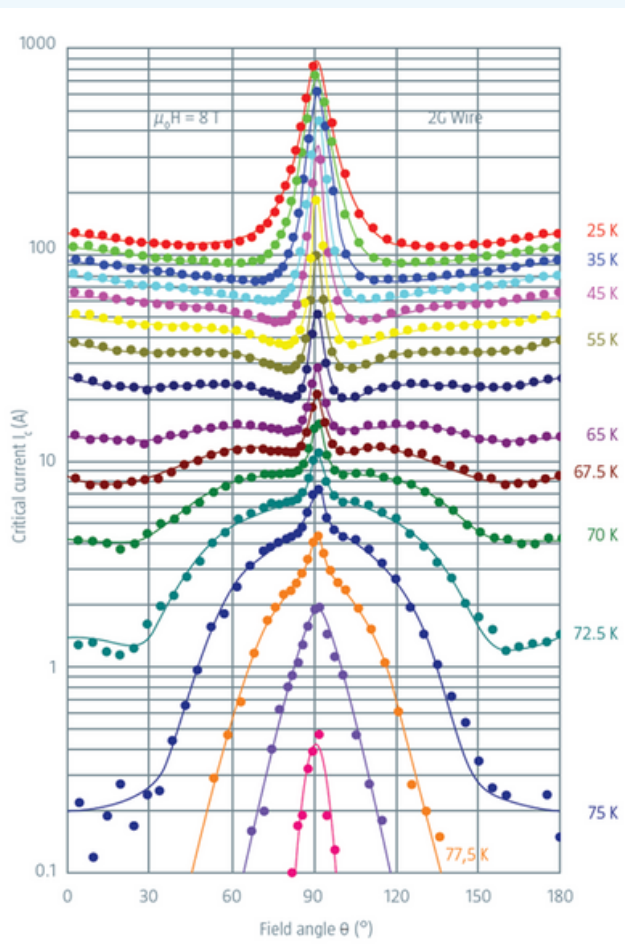

Standard system includes

- Magnet subsystem with integrated cryocooler
- Active magnet protection electronics linked to integrated temperature sensors and voltage taps
- Magnet energy dump system
- Bipolar power supply for magnet
- Sample environment cooled with a flowing He gas circuit
- Sample rotation stage
- Sample temperature control (LakeShore 336)
- Sample current source to 1600 A

- Sample voltage preamplifier
- Field measurement incorporated in software
- Proven control software (in LabVIEW) for transport I_c measurement
- Sample probe
- 1 year warranty

System Specifications

- 5, 8, 12 T full-field options
- Magnet cool down (room temperature to operating temperature) <60 h
- Sample cool down: 1 – 2 h
- Sample size: up to 12 mm x 120 mm x 3 mm as standard, nominal 10 mm voltage spacing
- Sample space: \varnothing 20 mm

System Requirements

- 50/60Hz 3P power for magnet and sample environment
- Helium gas supply required for sample exchange
- Vacuum pump for installation and maintenance; turbomolecular pump recommended with minimum pumping speed 40 l/s and ultimate pressure <10⁻⁷ mbar

System Options

- Calibrated field measurement system (LakeShore)
- I-V curve analysis software
- LabVIEW Licence
- Low maintenance vacuum pump
- Water chiller
- Lower capacity systems (field, sample temperature) available as options



HTS-110
1B Quadrant Drive, Waiwhetu
Lower Hutt 5010, New Zealand

+64 4 570 8880
info@hts-110.com
nz.linkedin.com/company/hts-110

